

# MRK HEALTHCARE PVT. LTD. IFU

### Ultra Gloves Beadless, Sterile Powdered

#### **DEVICE INTENDED USE:**

The surgical gloves are intended to act as a protective barrier between the patient and health care worker during invasive surgeries and also to facilitate general hand hygiene.

### DEVICE CATALOGUE NO. AND AVAILABLE SIZES:

Catalogue no.	Sizes.
ULTLPEBL	5.5,6.0,6.5,7.0,7.5,8.0,8.5,9.0

### **BASIC UDI:**

8905159SRGLPWCB

### **DEVICE DESCRIPTION:**

<u>Ultra Gloves Beadless - Sterile (Powdered Gloves)</u>

Ultra Gloves anatomically shaped medical gloves with the thumb positioned towards the palmer surface of the index finger rather than lyingflat and intended for surgery.

#### **INTENDED USER:**

This is used by surgeons, operation theatre staff and healthcare professional

#### TARGET PATIENT POPULATION:

Used for all patient population except in patients with known allergy to natural latex rubber.

### **DEVICE SHELF LIFE:**

5 years from the date of manufacture printed on the Product Label.

### **STORAGE INSTRUCTION:**

It is recommended to store the gloves in dry place, in the temperature of 5°C to 40°C and to protect them against direct sunlight.

#### METHOD OF STERILIZATION:

Device is supplied after EO (Ethylene Oxide) Sterilization.

### **INDICATIONS:**

Intended to be worn on the hands during medical surgical procedures to provide barrier against potentially infectious fluids and other contaminants.

### WARNINGS AND PRECAUTIONS:

- 1. Do not use after the expiry date printed on the label.
- 2. Do not use if the Package is opened or damaged. Use of product whose package is opened,

Rev.	С	Rev.	10/09/2022	Doc No:	MRK/IFU/SRG-	Page <b>1</b> of	Device	Ultra Gloves Beadles, Sterile
No.		Date			PD/S-08	5	Name	Powdered



MRK HEALTHCARE PVT. LTD. IFU

## Ultra Gloves Beadless, Sterile Powdered

or damage may cause inflammation.

- 3. After donning remove powder by wiping gloves thoroughly with a sterile wet sponge, sterile wet towel or other effective method.
- 4. Do not Re-sterilize The excess ETO residue which stays after re-sterilization may be toxic to the users and patients.
- 5. Do not Re Use The reuse of the gloves may cause severe complications such as cross contamination, dermatitis, loss of physical properties, Blood-Borne Infection, Post-operative wound infection, allergic reaction and poor barrier protection.
- 6. Latex gloves are made of Natural rubber latex, which may cause allergic reactions including Latex Allergy Anaphylactic if the user is allergic to latex.
- 7. Gloves may contain excess powder residues which may cause respiratory tract and pulmonary disease.
- 8. Single Use Packaging label and Sales Packaging Label.
- 9. Device should not be stored in direct sunlight
- 10. Device disposable should be done as per local regulatory. Failing to do so may lead to toxic to environment.
- 11. Sterility guaranteed until package is opened or damaged.

### **CONTRA INDICATIONS:**

- 1. Gloves contain Powder content, persons who are sensitive to powder may develop allergy towards the powder content
- 2. Latex gloves are made of Natural rubber latex, which may cause allergic reactions including Latex Allergy Anaphylactic if the user is allergic to latex.
- 3. Gloves contain Natural Latex; persons who are sensitive to Latex should consult a physician before using

### **DIRECTION FOR USE:**

- Select the appropriate size Gloves for the hand.
- Take out the Gloves from the pouch by peeling it off at the site of direction for open.
- Wear the gloves as left to the Left hand & Right to the Right Hand as denoted on the pouch.
- Must check the date of manufacturing and expiry date before use.
- Adjust the gloves as needed.

### A) How to Don Gloves:

- Rubbing the hand with alcohol or wash with water
- Dry hands before donning the gloves.
- Take out gloves from single unit packaging.
- Gloves need to be donned carefully; do not apply excessive force to pull the gloves when donning.
- Keep the fingernails short and change gloves frequently to avoid tearing issue.

### B) How to Remove Gloves:

- The gloves should be discarded with an appropriate waste disposal container after use according to local disposal regulations

No. Date PD/S-08 5 Name Powdered	Rev.	С	Rev.	10/09/2022	Doc No:	MRK/IFU/SRG-	Page <b>2</b> of	Device	Ultra Gloves Beadles, Sterile
	No.		Date			PD/S-08	5	Name	Powdered



MRK HEALTHCARE PVT. LTD.

# IFU

## Ultra Gloves Beadless, Sterile Powdered

### **DURATION OF USE:**

Duration of Use is short term use (< 24 hours)

### MEDICAL BENEFITS:

- NRL gloves are competent barrier to protect against infections for both healthcare professionals ٠ and the patients.
- NRL gloves provide lower rates of perforation and lower viral leakage rates. •
- NRL gloves are easy to put on comfortable to wear and provide adequate, durable protection.
- NRL gloves have good barrier integrity.
- NRL gloves have less after-use defects.
- NRL Gloves has significant greater satisfaction with regard to factors such as quality, safety and • durability.
- NRL gloves have high tear propagation strength. •
- NRL gloves have low perforation rate. •
- NRL gloves have high tensile strength.
- NRL gloves have good fit and comfort.

### SIDE EFFECTS:

Latex Allergy, Surgical site infection, Inflammation, Allergy, Pain, Rashes, Itching, Peeling of skin, Hypersensitivity type-I reaction, Skin redness, Ulcerated skin

Rev. No.	С	Rev. Date	10/09/2022	Doc No:	MRK/IFU/SRG- PD/S-08	Page <b>3</b> of <b>5</b>	Device Name	Ultra Gloves Beadles, Sterile Powdered
-------------	---	--------------	------------	---------	-------------------------	------------------------------	----------------	---




MRK HEALTHCARE PVT. LTD.

# Ultra Gloves Beadless, Sterile Powdered

IFU

SYMBO	LS USED IN DEVI		PACKAGING AN	D SALES PACKA	GING
	Manufacturer		Date of Manufacture		Keep away from Sunligh
EC REP	Authorized Representative in the European Community/ Authorized representative European Union		Use by Date/ Expiry Date	Ť	Keep Dry
	Contains presence of Natural Rubber Latex	LOT	Batch Code	(2)	Do not Re-use
STERILEEO	Sterilized using Ethylene Oxide		Do not use if package is damaged and consult instructions for use	Â	Caution
STERRAIZE	Do not resterilize	MD	Medical Device	UDI	Unique Device Identifier
	Single sterile barrier system with protective packaging inside	<b>CE</b> 2460	CE Mark Symbol with notified body number	5°C 40°C	Storage Temperatur e
QTY. 2N (1PAIR)	No: of gloves in the package				
-	entative and com	petent authority	ufacturer (MRK Healt of the member state	-	ent is
Rev. C Rev. No. Date	10/09/2022 Doc No:	MRK/IFU/SRG-	Page 4 of Device	Ultra Gloves Beadles	s, Sterile

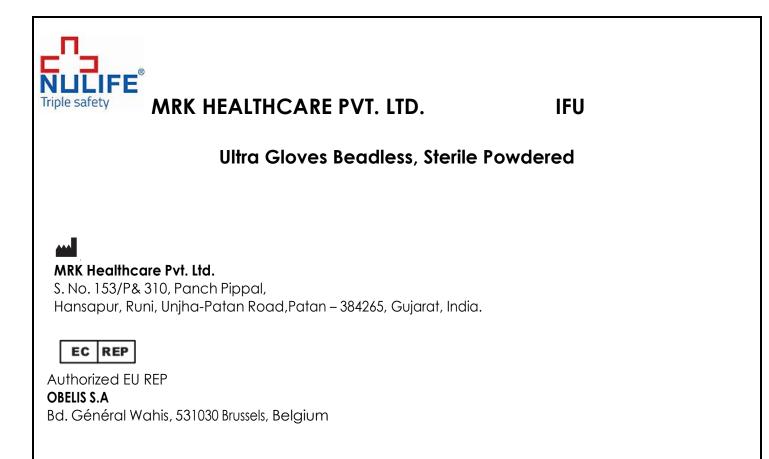

# **Revision History**

Rev. No.	Date	Reason for Revision				
Α	20/04/2022	Initial Release				
В	09/08/2022	Sterile & Nonsterile segregated as per TR comments				
С	10/09/2022	Warning & precaution updated with residual risk as per TR comments				

Rev. No.	С	Rev. Date	10/09/2022	Doc No:	MRK/IFU/SRG- PD/S-08	Page <b>5</b> of <b>5</b>	Device Name	Ultra Gloves Beadles, Sterile Powdered
					/	-		